



Doclet No. 15-XZ-4971

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

#5  
4-12-02

IN THE APPLICATION OF:

Kenneth Kump

Serial No.: 09/344,190

Filed: 6/24/1999

For: METHOD AND APPARATUS FOR  
DETERMINING A DYNAMIC RANGE  
OF A DIGITAL MEDICAL IMAGE

) EXPRESS MAIL NO. EL649151360US  
)  
)

) DATE: April 9, 2002  
)  
)

) Examiner: B. Choobin  
)  
)

) Group Art Unit: 2621  
)

RECEIVED

APR 12 2002

Technology Center 2600

Dear Sirs:

Please substitute the attached proposed drawing sheets for Figs. 2 and 7 to delete the downward arrow from final steps 66 and 212, respectively, and Fig. 4 to correctly label left side 77 and right side 79. The proposed drawing changes do not add new matter.

Respectfully submitted,  
McANDREWS, HELD & MALLOY, LTD.


Date: April 9, 2002

By:

Dean D. Small  
Reg. No. 34,730  
Attorney for Applicant

McANDREWS, HELD & MALLOY, LTD.  
500 West Madison Street  
Chicago, Illinois 60661  
Telephone: (312) 707-8889

Fig. 2

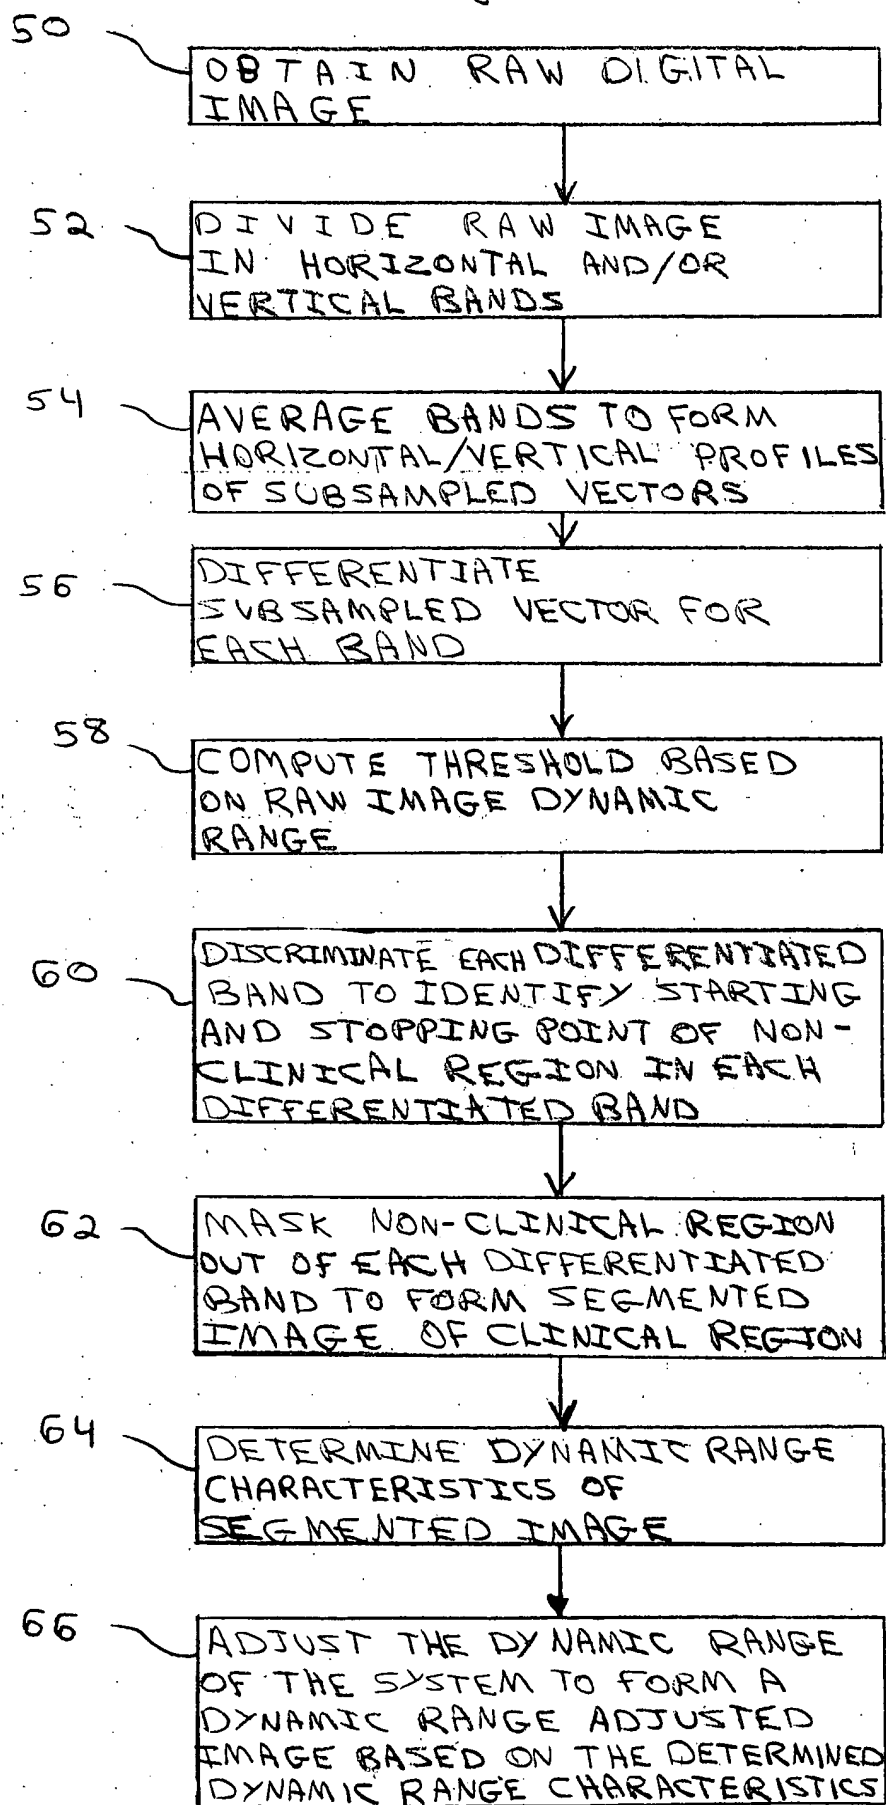



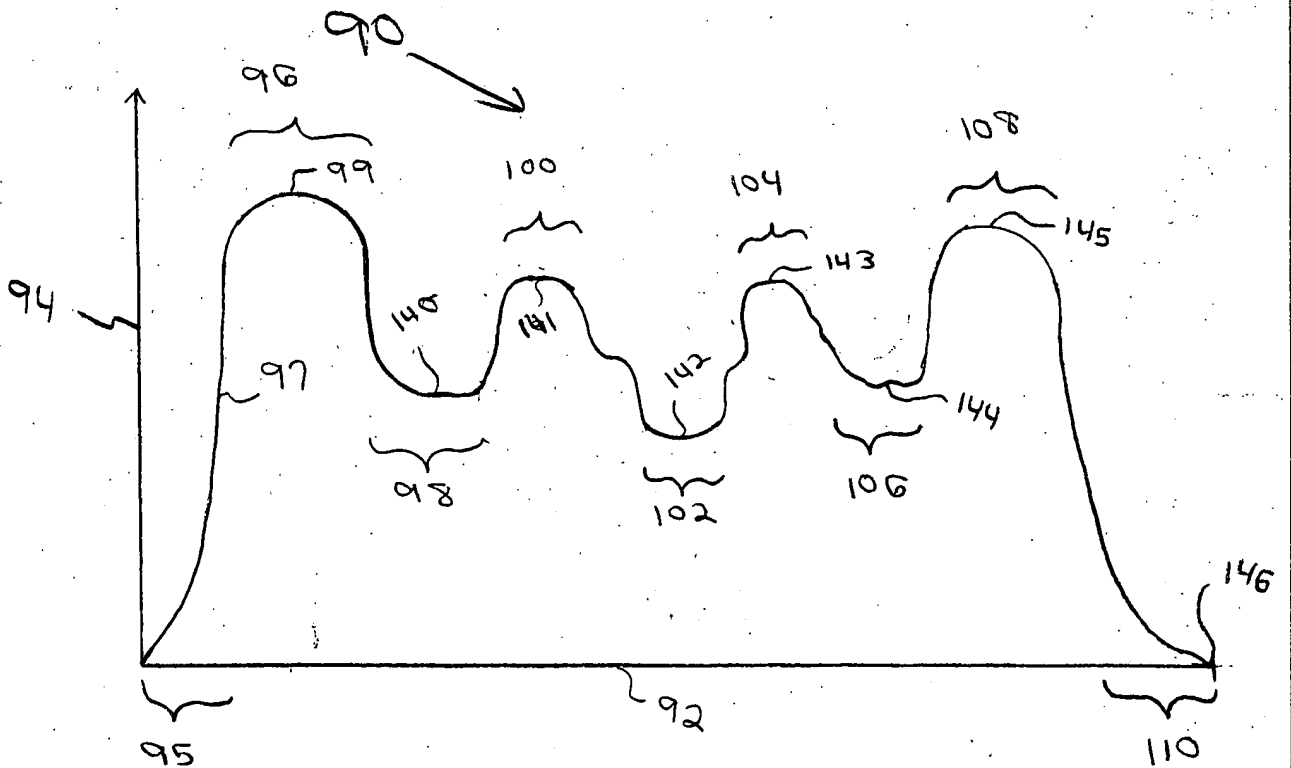


Fig. 7

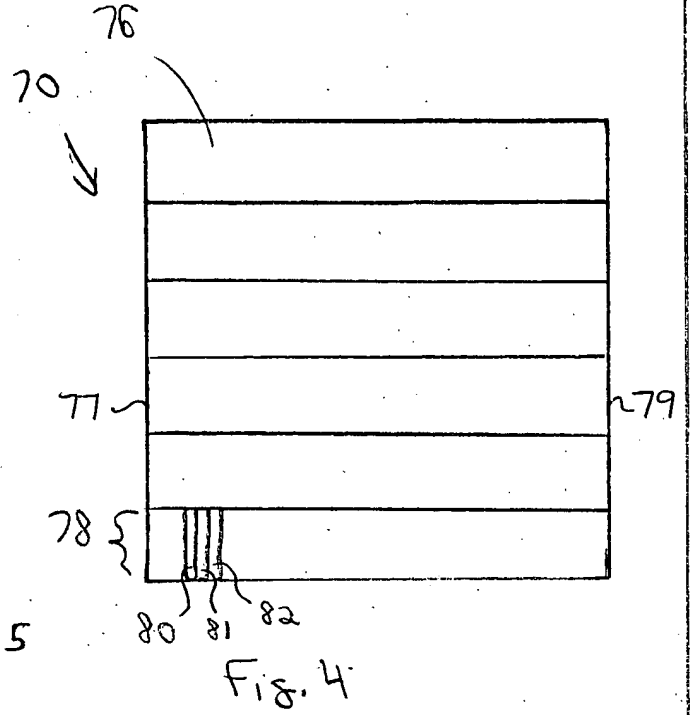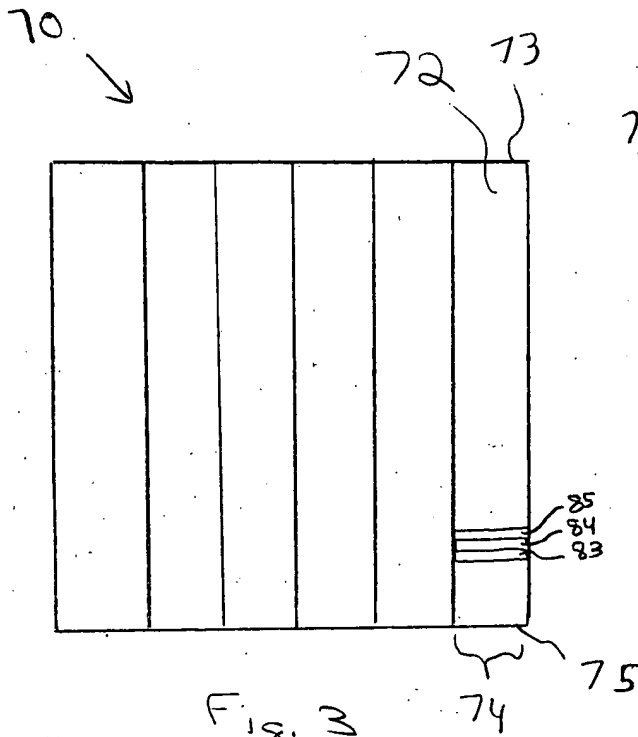